

Installation Guide for Lantronix XPort03/04 and XPort05 Firmware

Introduction

This document will go through the steps required to update the LANTRONIX XPORT-03/-04/-05.

****NOTE: XPORT03/04 is only compatible with CIC949-1V1.1 and XPORT 05 is only compatible with CIC949-2V1.5.****

Equipment Requirements

- Power supply with –LAN option hardware installed.
- LAN Cable
- Lantronix Server Configuration Utility version 4.2.0.4 or higher.

Software found here: <http://www.lantronix.com/device-networking/utilities-tools/device-installer.html>

Setup

1. Turn ON Power Supply.
2. Connect the power supply LAN to computer or to the Network.
3. Open LANTRONIX device installer program. Figure 1 will appear. Identify the XPORT, that required configuration, from the listed of items by its Hardware Address.
4. Highlight the item that needs update. ****Note if the file is XPort03/04 or XPort05.****

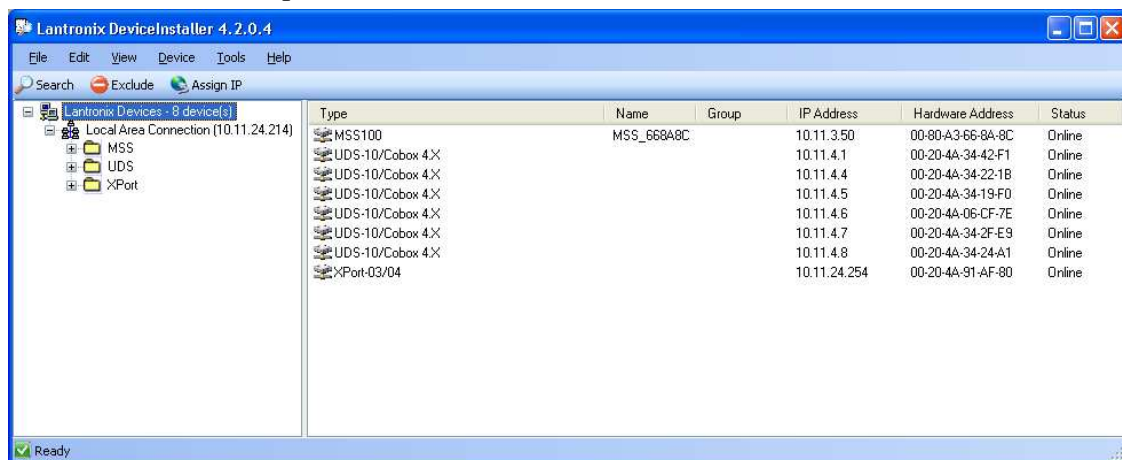


Figure 1: Device installer screen

Configuration

5. While the item is highlighted, select upgrade from the top menu. Figure 2 will appear.

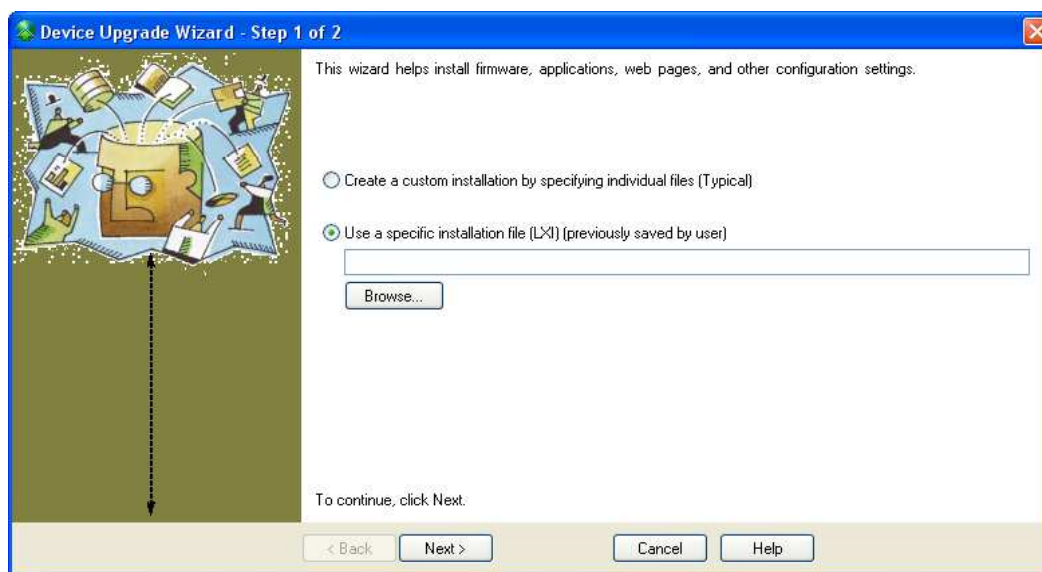
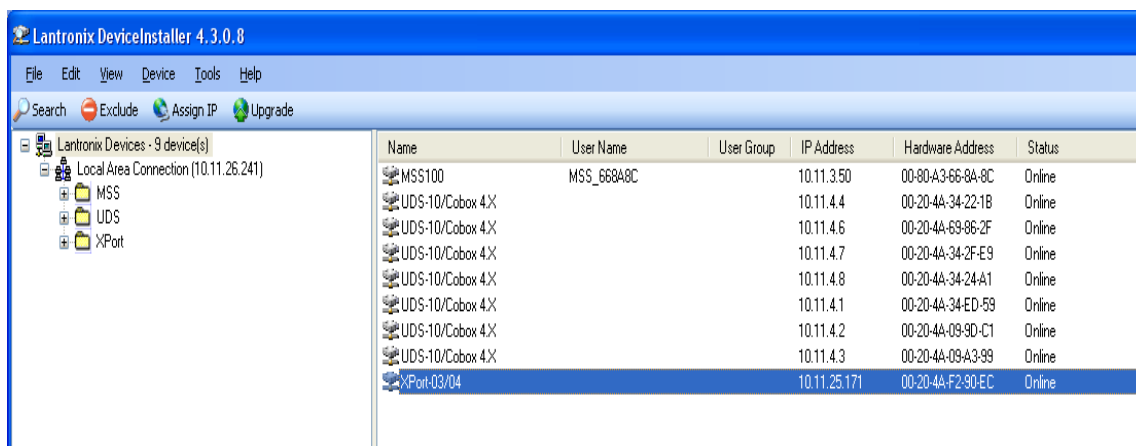


Figure 2: Device Upgrade Screen

6. Select “Use specific installation file” and click “Browse”.

7. If upgrading XPort 03/04 navigate to zip file downloaded “cic949-1r1.1.zip” and select the file “CIC949-1rev1.1.lxi”.

If upgrading XPort05 navigate to the zip folder “CIC949-2V1_5.zip” and select the file “CIC949-2V1.5.lxi”.

These are the current file revisions and could change with upgrade. Click Next. Figure 3 will appear and the update sequence will take place.

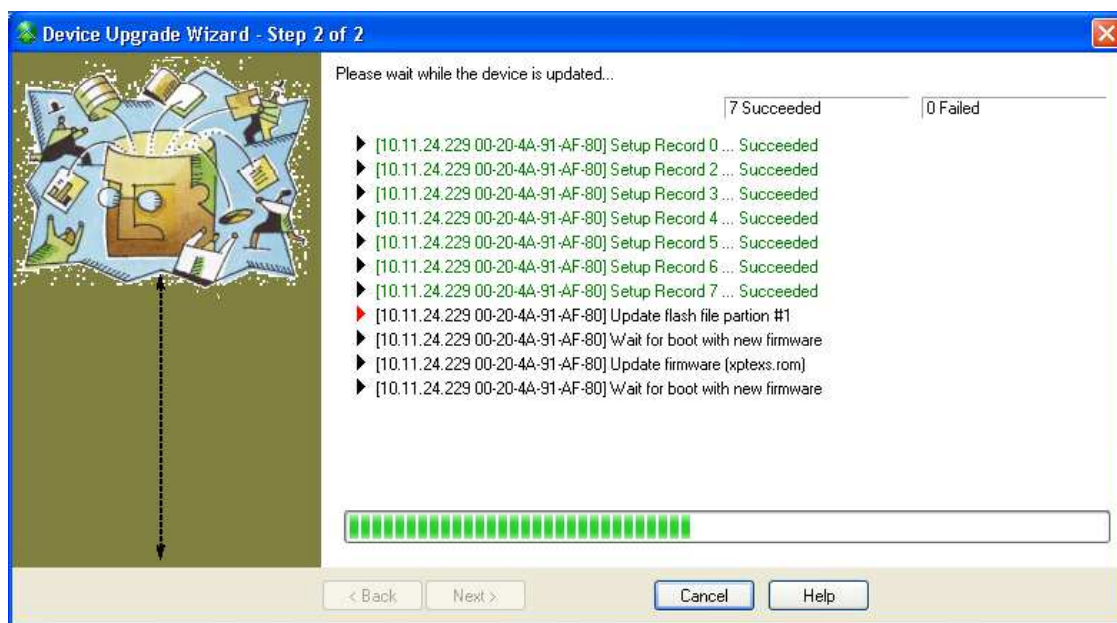


Figure 3:Update Sequence screen

Verify all the download sequences show as “Succeeded”.

Update complete.

California Instruments Product Support:

On-Line Request:

www.programmablepower.com/support/support_CallInst.htm

Direct: ci.ppd@ametek.com

Phone: 800-733-5427