

Evaluation Board User Guide UG-125

One Technology Way • P.O. Box 9106 • Norwood, MA 02062-9106, U.S.A. • Tel: 781.329.4700 • Fax: 781.461.3113 • www.analog.com

Setting Up the Evaluation Board for the ADCLK944

PACKAGE CONTENTS

Evaluation board with ADCLK944 component installed

GENERAL DESCRIPTION

This user guide describes how to set up and use the evaluation board for the ADCLK944. The ADCLK944 data sheet should be used in conjunction with this user guide.

The data sheet contains full technical details about the specifications and operation of this device.

The ADCLK944 is a very high performance clock fanout buffer. The evaluation board is fabricated using high quality Rogers dielectric material. Transmission line paths are kept as close to 50 Ω as possible.

DIGITAL PICTURE OF EVALUATION BOARD

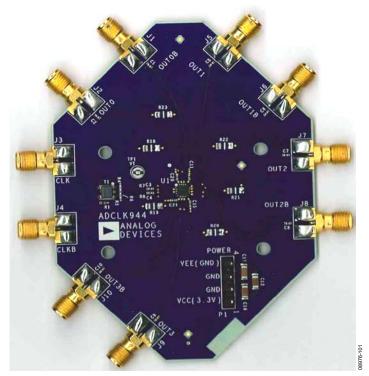


Figure 1. ADCLK944 Evaluation Board

UG-125

Evaluation Board User Guide

TABLE OF CONTENTS

Package Contents1	Evaluation Board Hardware	3
General Description1	Recommended Board Setup	3
Digital Picture of Evaluation Board1	Clock Outputs	
Revision History	Evaluation Board Schematic and Artwork	5

REVISION HISTORY

4/10—Revision 0: Initial Version

EVALUATION BOARD HARDWARE

RECOMMENDED BOARD SETUP

The recommended setup for the ADCLK944 evaluation board is shown in Figure 2. $V_{\rm CC}$ is set to 2.5 V to 3.3 V, and $V_{\rm EE}$ is set to GND.

On the evaluation board, the clock input is set up for single-ended-to-differential operation via the balun. In addition, series capacitors in the path provide ac-coupled inputs to the ADCLK944. The common-mode voltage for both inputs is provided by tying V_{REF} and V_{T} together. This connection is made with R13 installed at the factory.

The range of the peak-to-peak input voltage swing at CLK is 0.2 V p-p to 1.7 V p-p. Note that output jitter performance is degraded by an input slew rate, as shown in the ADCLK944 data sheet.

Table 1. Basic Equipment Required

Quantity	Description
1	Single power supply
1	Signal source
1	High bandwidth oscilloscope
4	Matched high speed cables

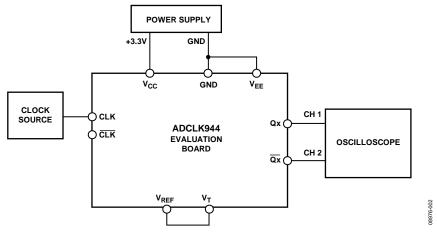


Figure 2. Recommended Setup for Device Evaluation

CLOCK OUTPUTS

The ADCLK944 has four differential outputs. All differential clock outputs on the evaluation board are biased to GND via 200 Ω and ac-coupled to the SMAs. From the SMAs, use matched 50 Ω coaxial cables into the oscilloscope for evaluation. See the evaluation board schematic in Figure 4 for more details.

Table 2. Power Connections via P1

Label	ADCLK944
GND	Connect to GND
V_{CC}	Connect to 3.3 V
V _{EE}	Connect to GND




Figure 3. ADCLK944 1:4 Clock/Data Buffer Block Diagram

EVALUATION BOARD SCHEMATIC AND ARTWORK

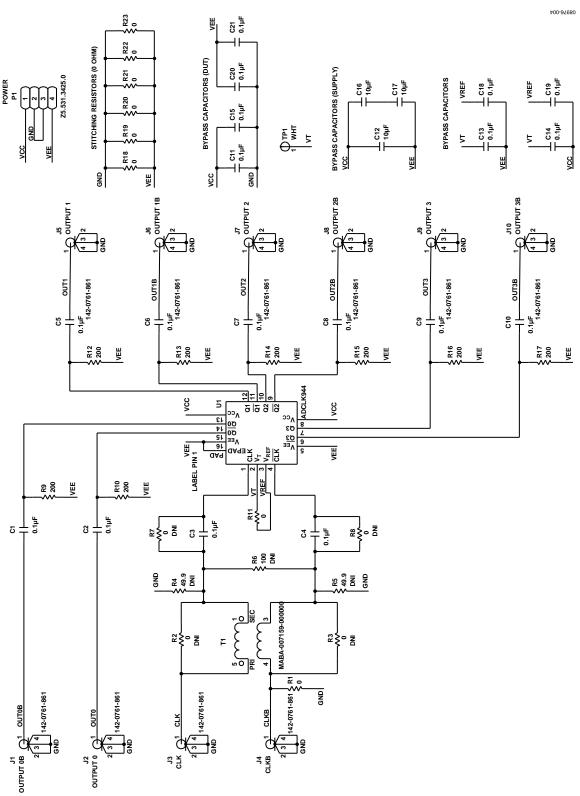


Figure 4. ADCLK944 Evaluation Board Schematic

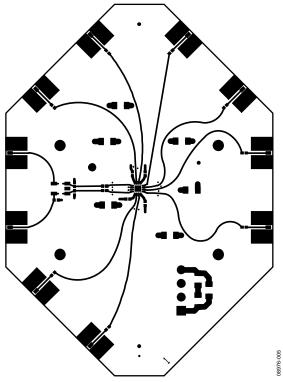


Figure 5. Top Trace Layer

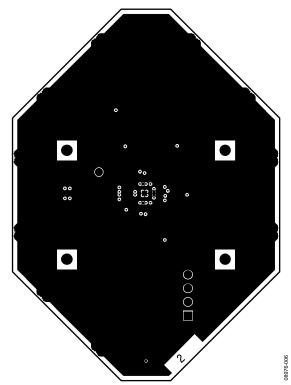


Figure 6. Ground Plane Layer

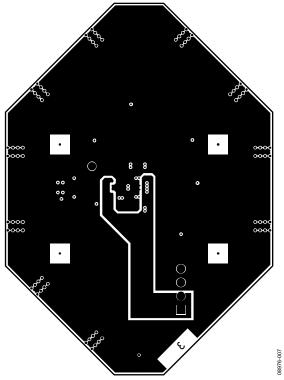


Figure 7. V_{CC} and V_{EE} Power Plane Layer

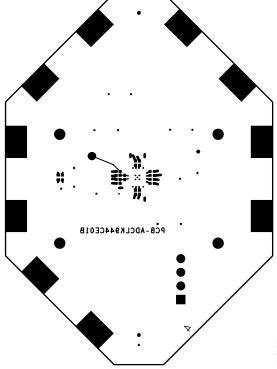


Figure 8. Bottom Trace Layer

UG-125

Evaluation Board User Guide

NOTES



ESD Caution

ESD (electrostatic discharge) sensitive device. Charged devices and circuit boards can discharge without detection. Although this product features patented or proprietary protection circuitry, damage may occur on devices subjected to high energy ESD. Therefore, proper ESD precautions should be taken to avoid performance degradation or loss of functionality.

Legal Terms and Conditions

By using the evaluation board discussed herein (together with any tools, components documentation or support materials, the "Evaluation Board"), you are agreeing to be bound by the terms and conditions set forth below ("Agreement") unless you have purchased the Evaluation Board, in which case the Analog Devices Standard Terms and Conditions of Sale shall govern. Do not use the Evaluation Board until you have read and agreed to the Agreement. Your use of the Evaluation Board shall signify your acceptance of the Agreement. This Agreement is made by and between you ("Customer") and Analog Devices, Inc. ("ADI"), with its principal place of business at One Technology Way, Norwood, MA 02062, USA. Subject to the terms and conditions of the Agreement, ADI hereby grants to Customer a free, limited, personal, temporary, non-exclusive, non-sublicensable, non-transferable license to use the Evaluation Board FOR EVALUATION PURPOSES ONLY. Customer understands and agrees that the Evaluation Board is provided for the sole and exclusive purpose referenced above, and agrees not to use the Evaluation Board for any other purpose. Furthermore, the license granted is expressly made subject to the following additional limitations: Customer shall not (i) rent, lease, display, sell, transfer, assign, sublicense, or distribute the Evaluation Board; and (ii) permit any Third Party to access the Evaluation Board. As used herein, the term "Third Party" includes any entity other than ADI, Customer, their employees, affiliates and in-house consultants. The Evaluation Board is NOT sold to Customer; all rights not expressly granted herein, including ownership of the Evaluation Board, are reserved by ADI. CONFIDENTIALITY. This Agreement and the Evaluation Board shall all be considered the confidential and proprietary information of ADI. Customer may not disclose or transfer any portion of the Evaluation Board to any other party for any reason. Upon discontinuation of use of the Evaluation Board or termination of this Agreement, Customer agrees to promptly return the Evaluation Board to ADI. ADDITIONAL RESTRICTIONS. Customer may not disassemble, decompile or reverse engineer chips on the Evaluation Board. Customer shall inform ADI of any occurred damages or any modifications or alterations it makes to the Evaluation Board, including but not limited to soldering or any other activity that affects the material content of the Evaluation Board. Modifications to the Evaluation Board must comply with applicable law, including but not limited to the RoHS Directive. TERMINATION. ADI may terminate this Agreement at any time upon giving written notice to Customer. Customer agrees to return to ADI the Evaluation Board at that time. LIMITATION OF LIABILITY. THE EVALUATION BOARD PROVIDED HEREUNDER IS PROVIDED "AS IS" AND ADI MAKES NO WARRANTIES OR REPRESENTATIONS OF ANY KIND WITH RESPECT TO IT. ADI SPECIFICALLY DISCLAIMS ANY REPRESENTATIONS, ENDORSEMENTS, GUARANTEES, OR WARRANTIES, EXPRESS OR IMPLIED, RELATED TO THE EVALUATION BOARD INCLUDING, BUT NOT LIMITED TO, THE IMPLIED WARRANTY OF MERCHANTABILITY, TITLE, FITNESS FOR A PARTICULAR PURPOSE OR NONINFRINGEMENT OF INTELLECTUAL PROPERTY RIGHTS. IN NO EVENT WILL ADI AND ITS LICENSORS BE LIABLE FOR ANY INCIDENTAL, SPECIAL, INDIRECT, OR CONSEQUENTIAL DAMAGES RESULTING FROM CUSTOMER'S POSSESSION OR USE OF THE EVALUATION BOARD, INCLUDING BUT NOT LIMITED TO LOST PROFITS, DELAY COSTS, LABOR COSTS OR LOSS OF GOODWILL. ADI'S TOTAL LIABILITY FROM ANY AND ALL CAUSES SHALL BE LIMITED TO THE AMOUNT OF ONE HUNDRED US DOLLARS (\$100.00). EXPORT. Customer agrees that it will not directly or indirectly export the Evaluation Board to another country, and that it will comply with all applicable United States federal laws and regulations relating to exports. GOVERNING LAW. This Agreement shall be governed by and construed in accordance with the substantive laws of the Commonwealth of Massachusetts (excluding conflict of law rules). Any legal action regarding this Agreement will be heard in the state or federal courts having jurisdiction in Suffolk County, Massachusetts, and Customer hereby submits to the personal jurisdiction and venue of such courts. The United Nations Convention on Contracts for the International Sale of Goods shall not apply to this Agreement and is expressly disclaimed.

©2010 Analog Devices, Inc. All rights reserved. Trademarks and registered trademarks are the property of their respective owners. UG08976-0-4/10(0)



www.analog.com